


Sterile Processing Guide

GloShield™

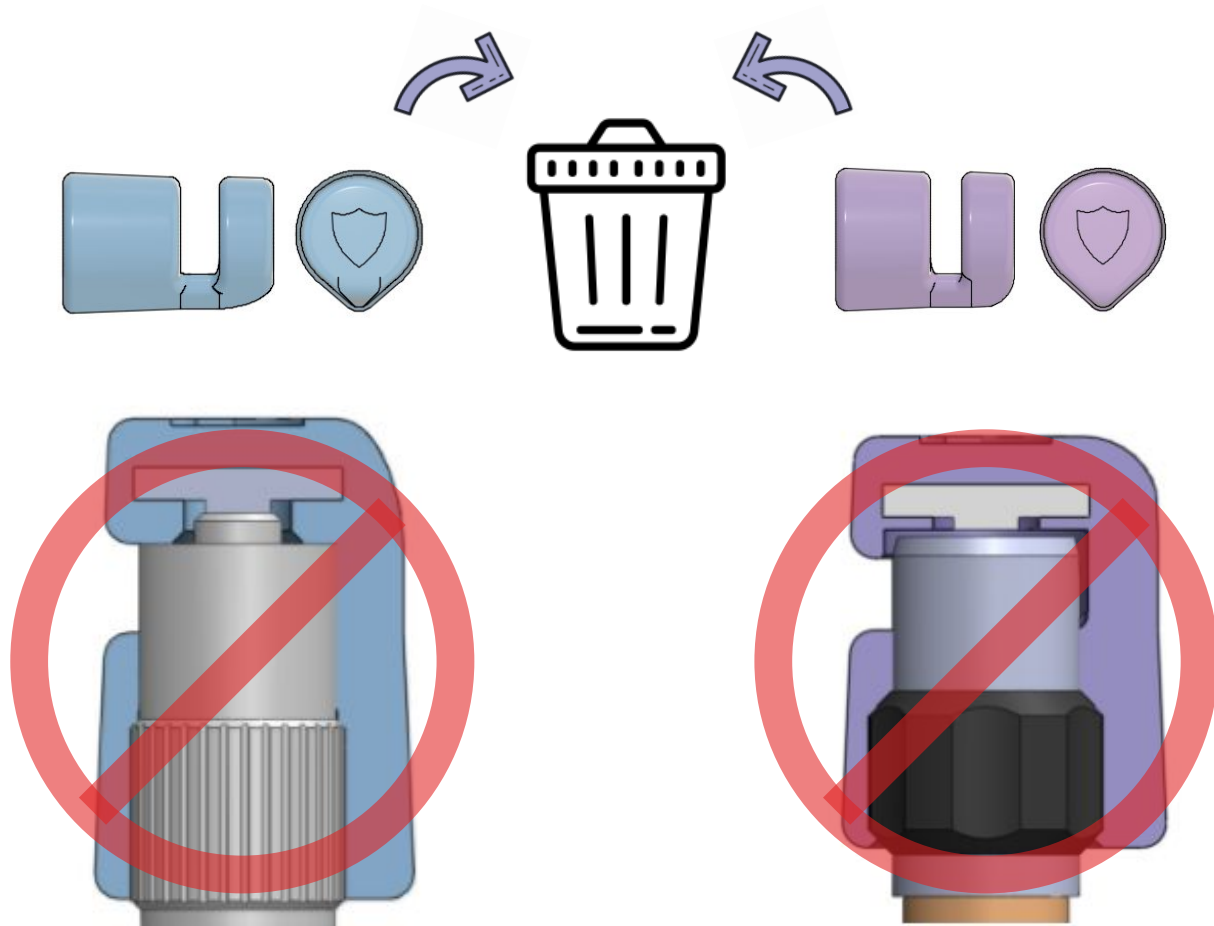

CHECK each light cable connector prior to reesterilization.

If you see a GloShield connected to a light cable or in a tray,
DISCONNECT GloShield and **DISCARD**.

GloShield is a disposable item; **DO NOT RESTERILIZE**.